arXiv:1209.5250v1 [cond-mat.soft] 24 Sep 2012

A new tuning fork-based instrument for oscillatory shear rheology of nano-confined liquids

Karan Kapoor[1], Vinod Kanawade[1], Vibham Shukla[1] and Shivprasad Patil[1,a)]
[1] *Physics Division, Indian Institute of Science Education and Research, Pune 411008, Maharashtra, India*

We present a new method to measure rheological response of liquids confined to nano-scale which exhibit a considerable slow-down in dynamics compared to bulk liquids. The method relies on using a robust force sensor that has a sensitivity to measure shear forces in the range of 1 to 10 nN and a stiffness of 5.5×10^4 N/m to avoid thermal noise. Off-resonance operation ensures application of a range of shear frequencies . This range is higher than the inverse of the system's mechanical relaxation time and allows the measurement of non-linear effects emerging due to significant "slow down" in dynamics upon confinement. The instrument is a step forward towards resolving the controversies about the nature of nano-confined liquids.

I. INTRODUCTION

The role of nano-confined liquids in many areas ranging from tribology to biology is universally accepted [1–4]. Such confinement by solid walls induces significant alteration in their physical properties such as diffusion coefficient [6] and viscosity[7, 8], furthermore the liquid possibly undergoes solidification [7, 9]. However, the details of this change in behaviour have been argued upon ever-since the pioneering experiments that measured oscillatory solvation forces on liquids confined to molecular-level thickness [10–12]. In particular, the measurement of viscosity of confined liquid using different experimental approaches have led to contradictory results [13, 15–18]. The Surface Force Apparatus(SFA) measurements have reported that a hydrogen-bonded liquid like water shows no change in viscosity upon confinement down to 4 nm and below[17, 18], whereas other non-associative fluids such as Octamethylcyclotetrasiloxane(OMCTS) exhibit significant solidification upon confinement[9]. However, many other measurements of shear viscosity of nano-confined water using SFA and Atomic Force Microscope(AFM) have reported orders of magnitude increase in viscosity under confinement[7, 8]. Recently both the shear and normal measurements performed using AFM have suggested that the relaxation time of nano-confined water films is orders of magnitude more than that of bulk water[19, 20].

The fluid volume involved in the viscosity measurement of nano-confined liquids is of the order of atto-litres to zepto-litres, and the shear forces that they generate are of the order of nN. Therefore conventional rheology instruments are not capable of revealing the rich non-linear behaviour of these films. SFA and AFM set-ups are modified to measure the shear stress developed due to straining of nano-confined thin films. In both SFA and AFM experiments the shear frequency is limited from a few Hz to 1 KHz. In order to measure the change in relaxation time upon confinement we need a wider shear frequency range, typically larger than the inverse of the system's relaxation time. Also jump-to-contact instability of the confining surfaces is a serious issue in controlling the film thickness while shear straining these films. It is therefore important to develop new techniques employing force sensors which have large normal stiffness to avoid the instability and can perform in wider shear frequency range with force sensitivity of the order of nN. This paper reports the development of an instrument for oscillatory rheology on nano-confined liquids with unprecedented shear frequencies and near infinite normal stiffness. We also develop the necessary analysis method to quantify relaxation time of the nano-confined liquid.

The new instrument proposed in this paper employs tuning fork as a shear force sensor in rheology of nanoconfined liquids. Quartz crystal tuning fork is a commonly available device used as time-keeping element in watches. In recent years quartz tuning fork has been used as a robust force sensor in AFM with low signal to noise ratio due to its high quality factor of resonance and very high stiffness compared to conventional AFM cantilevers[21–24]. Tuning fork has not been used so far to measure shear response of nano-confined liquids since the charge accumulated due to strain on its electrode surface is used to measure the the bending of the arms. This is difficult to measure it liquid environment. We use tuning fork as shear stress measuring force sensor by keeping it outside the liquid and mounting a fibre with a tip on one of its arms. The tip is immersed in liquid and the tuning fork is used to measure the stress on the fibre tip by measuring the difference in current through the arms. The amplitude and phase measurement is related to shear stress and the complex damping coefficient by modelling the fibre-tuning fork system as two elastically coupled oscillators and solving the resulting differential equation.

---

a) Corresponding author: s.patil@iiserpune.ac.in

The paper is organized in the following manner. We first discuss the feasibility of using tuning forks for shear measurements in nano-confined water followed by the theory and modelling required to quantify the experimental data. We describe the design and development of the instrument and finally present initial results on nano-confined water using the instrument.

II. OFF-RESONANCE TUNING FORK FOR NANO-RHEOLOGY

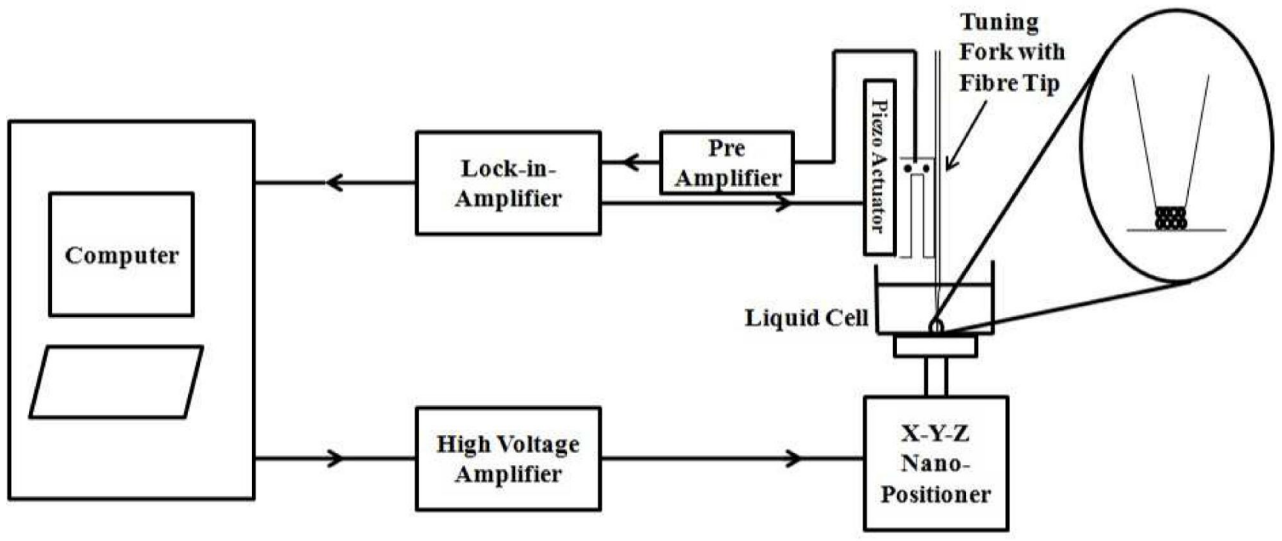

FIG. 1: Schematic of the Experimental set-up

Figure 1 describes the tuning fork as a proposed force sensor in measurement of rheological response of nano-confined liquid. A fibre with a sharp tip at its end is attached to the free arm of the tuning fork. It extends further from the arm to immerse itself in the liquid. We oscillate one arm of the tuning fork using a piezoelectric crystal. The resulting amplitude of the second arm is measured using a lock-in amplifier. The change in this amplitude upon bringing the tip close to the substrate placed at the bottom of the liquid cell is a measure of shear stress generated in the film; while phase gives us information about the nature of the nano-confined liquid, namely solid-like, liquid-like or non-Newtonian fluid-like.

If the viscosity of the nano-confined liquid remains unchanged compared to its bulk value, the amplitude should not change upon approach. If the amplitude reduces upon approach but there is no phase change from the bulk value, then the film is more viscous but still Newtonian. A change in both the phase and amplitude suggests a non-Newtonian behaviour. Next we discuss the technical aspects of quantifying the experimental data.

In most applications involving tuning fork as a force sensor, whether AFM imaging [23, 24] or force measurements during atom manipulations[25], it is driven on resonance. An atomically sharp tip is mounted on its free arm. It is important to keep the tip mass minimal in order to avoid serious loading effects by the tip itself. Secondly, the dimensions of the tip are chosen such that the spring constant of the tip is orders of magnitude higher than that of the tuning fork and the tip bending is negligible compared to that of the tuning fork arm. The shift in the resonance frequency due to interaction between the tip and substrate is measured and is used as feedback control parameter in imaging. The shift itself is related to interaction stiffness if the amplitude is small enough compared to the interaction length scale[25]. However in our application the tip length is significant owing to the fact that the tuning fork remains outside the liquid. Secondly, in order to perform shear rheology we need to perform measurements in a range of frequency, at least covering one or two decades around the inverse of longest relaxation time the film may possess. Therefore we can not restrict ourselves to resonance. In this section we describe the feasibility of using tuning forks off resonance with a fibre tip having a lower stiffness than the tuning fork arm itself.

A. Off-resonance operation

First we discuss the issue of how to perform measurements in the sub resonance regime. Below resonance the two arms of tuning fork move in the same direction and the potential drop across the electrodes is expected to be zero. We performed finite element analysis simulation of the tuning fork driven below resonance in the range of 2 to 20 KHz using COMSOL. Figure 2 shows the bending in the arms when driven off resonance at frequency of 10 KHz. Clearly, there is excess bending in the free arm compared to the one mounted on the piezo-crystal and the phase lag between the arms is zero. We argue that this extra bending emerges due to inertia. This signal is the measure of shear strain amplitude. Experimentally when a tuning fork is driven below resonance, there is indeed a measurable signal that arises due to the difference in the current through the two electrodes. Typically with gain of 10^7, this difference results in 100mV signal in lock-in amplifier which corresponds to roughly 20nm of free arm amplitude. This is discussed in more detail in later sections.

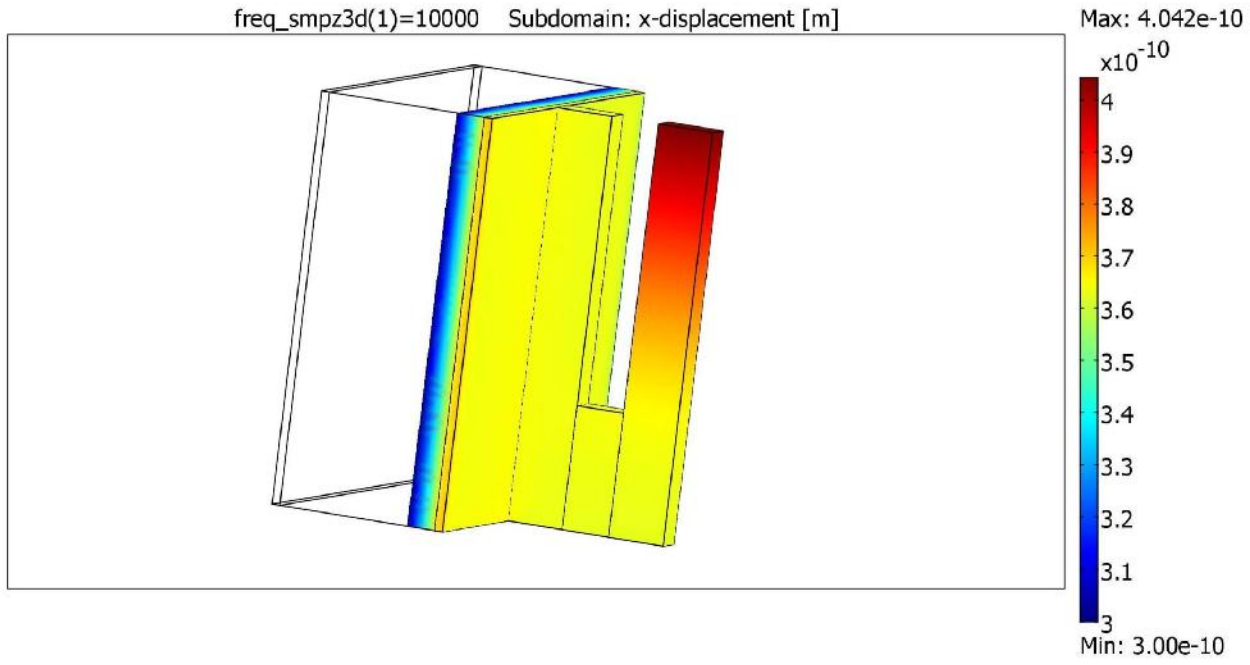

FIG. 2: Finite element analysis Simulation of the tuning fork and piezo arrangement at off-resonance frequency using COMSOL.One arm of the fork is oscillated at 10KHz with amplitude of 0.36nm. The amplitude of the free arm is more by 10%

B. Modelling of the shear force sensor

In oscillatory shear rheology, the phase lag between a sinusoidally varying strain and resulting stress is used for measurement of linear viscoelasticity of complex liquids. Typically for purely elastic response the stress is in phase with the strain whereas for purely viscous response the phase difference is 90 degrees. For viscoelastic materials the phase is between these two extremes . The shear stress is related to shear strain through the relation $\sigma = G^{*}\gamma$, where σ is shear stress, G^{*} is complex modulus and γ is shear strain. The storage (elastic) modulus G', and loss (viscous) modulus G'' is defined as $G^{*} = G' + iG''$, where i is an imaginary number. The relaxation time of linear viscoelastic system is $\tau = (G'/G'').1/\omega$ [26]. The complex viscosity is defined as $\eta = \eta' - i\eta''$.

From the foregoing discussion it is clear that in order to measure non-linear behaviour of the nano-confined liquid, it is crucial to measure the stress due to applied strain and their phase relationship. The shearing tip experiences a stress once it is immersed in bulk liquid. Our goal is to measure the change in this oscillatory stress upon confinement of liquid by the tip and its phase relationship with the strain. This is straightforward if we measure the change in amplitude of the tip with respect to its position from the surface. The phase can be measured with a lock-in amplifier.

It is noteworthy that in our measurement scheme the tip extending further from the tuning fork end has a stiffness k_2 which is much smaller than the tuning fork arm stiffness k_1. Ideally, the amplitude and phase at the end of the tip should be measured for rheological response of the confined liquid, but experimentally it is not possible. In our experiments the amplitude and phase are measured at the tuning fork arm and not at the end of the fibre. In order to measure viscoelastic response of nano-confined liquid film from experimentally observed tuning fork amplitude and phase, we require the development of a model for the the proposed force sensor. This theoretical treatment is different from previous such measurements using AFM and SFA. We model the tuning fork and the attached fibre as a system of two coupled springs. Figure 3 describes this modelling in detail. We seek the relationship between the phase at the tuning fork arm and the quantities k_1, k_2, L_1, L_2,γ,where γ is the damping coefficient.

The differential equations for the coupled system are

$$m_1\ddot{x_1} = A_0\sin(\omega t) - k_1(x_1 - L_1) + k_2(x_2 - x_1 - L_2) \tag{1}$$

$$m_2\ddot{x_2} = -\gamma\dot{x_2} - k_2(x_2 - x_1 - L_2) \tag{2}$$

where A_0 is the amplitude of the driving force, L_1, L_2 are equilibrium lengths of the two springs. γ is the damping coefficient of the liquid and x_1, x_2 are the instantaneous tuning fork arm and tip positions respectively.
Taking the solutions of the form:

$$x_1 = A_1e^{i\omega t} \qquad x_2 = A_2e^{i\omega t}$$

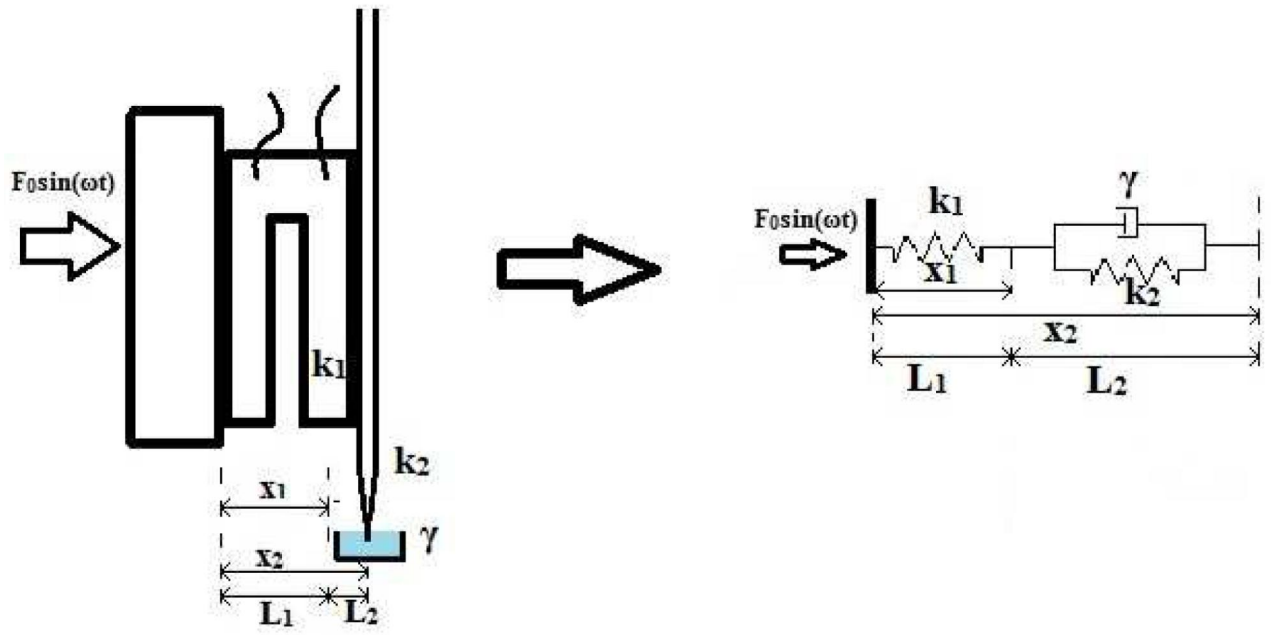

FIG. 3: The model of the tuning fork and the fibre. The fibre and the tuning fork arm are treated as springs with stiffness k_2 and k_1 respectively. The damping coefficient γ is provided by the liquid in which the tip is immersed. L_1 and L_2 are the equilibrium lengths of the two springs.

we get the equations in the matrix form as:

$$\begin{bmatrix} -m_1\omega^2 + k_1 + k_2 & -k_2 \\ -k_2 & -m_2\omega^2 + i\gamma\omega + k_2 \end{bmatrix} \begin{bmatrix} x_1 \\ x_2 \end{bmatrix} = \begin{bmatrix} A_0 \sin(\omega t) + k_1 L_1 - k_2 L_2 \\ k_2 L_2 \end{bmatrix} \tag{3}$$

Using LU decomposition, we obtain the solutions as:

$$x_1 = \frac{A_0 \sin(\omega t)(k_2 + i\gamma\omega - m_2\omega^2) + (i\gamma\omega - m_1\omega^2)(k_1L_1 - k_2L_2) + k_1k_2L_1}{k_2(k_1 - m_1\omega^2) - m_2\omega^2(k_1 + k_2 - m_1\omega^2) + i\gamma\omega(k_1 + k_2 - m_1\omega^2)} \tag{4}$$

$$x_2 = \frac{k_2A_0 \sin(\omega t) + k_1k_2L_1 + k_1k_2L_2 - k_2L_2m_1\omega^2}{k_2(k_1 - m_1\omega^2) - m_2\omega^2(k_1 + k_2 - m_1\omega^2) + i\gamma\omega(k_1 + k_2 - m_1\omega^2)} \tag{5}$$

To get the relationship for the phase difference between the oscillator and the tuning fork, as well as that between the oscillator and the fibre, we analyse the time dependent part of the solution of x_1 and x_2 :

$$\phi_1 = \tan^{-1}\left(\frac{-k_2^2\gamma\omega}{[(k_1 + k_2 - m_1\omega^2)(\gamma^2\omega^2 - m_2\omega^2(k_2 - m_2\omega^2)) + k_2(k_1 - m_1\omega^2)(k_2 - m_2\omega^2)]}\right) \tag{6}$$

$$\phi_2 = \tan^{-1}\left(\frac{\gamma\omega(k_1 + k_2 - m_1\omega^2)}{m_2\omega^2(k_1 + k_2 - m_1\omega^2) + k_2(k_1 - m_1\omega^2)}\right) \tag{7}$$

We plot ϕ_1 and ϕ_2 versus damping coefficient γ in figure 4. The phase of fibre tip, ϕ_2 immersed in liquid quickly takes the value of 90 degrees for damping coefficient of 0.1. This is a typical value of γ obtained from water viscosity and the area of the fibre that is immersed in the liquid. ϕ_1 too converges to 0 degrees. As expected, the tuning fork arm which stays out of liquid remains in phase with the driver and the fibre tip immersed in Newtonian viscous liquid gives phase difference of 90 degrees. Our solutions for ϕ_1 and ϕ_2 thus give a familiar result and the solutions we have arrived at are consistent with the physical picture of conventional response of Newtonian liquids.

Solving for γ, equation 6 yields a complex damping coefficient for any value of ϕ_1 greater than 0.1 degrees. Figure 5 shows plots of real and imaginary part of damping coefficient γ versus ϕ_1. For a fixed geometry of the fibre moving inside the liquid, the damping coefficient γ is proportional to viscosity η. A complex damping coefficient means a complex viscosity. This is a remarkable result, since it allows us to measure the non-Newtonian response of the liquid, if any, from the measurement of ϕ_1. Indeed in our experiments when the fibre is lowered into the liquid from air, there is no change in ϕ_1. ϕ_1 starts to take values in the range of 0 to 5 degrees once the fibre tip reaches within a few nm from the substrate, indicating a non-Newtonian response of the nano-confined liquid. The experimentally measured phase difference ϕ_1 is used to calculate the real and imaginary part of damping coefficient, namely $\gamma^{'}$ and $\gamma^{''}$

The complex viscosity of non-Newtonian fluids is defined as $\eta^* = \eta^{'} - i\eta^{''}$ and the relaxation time as $\tau = (\eta^{''}/\eta^{'}).1/\omega$ [27].

The relaxation time in terms of real and imaginary part of γ is given by

$$\tau = (\gamma^{''}/\gamma^{'}).\frac{1}{\omega} \tag{8}$$

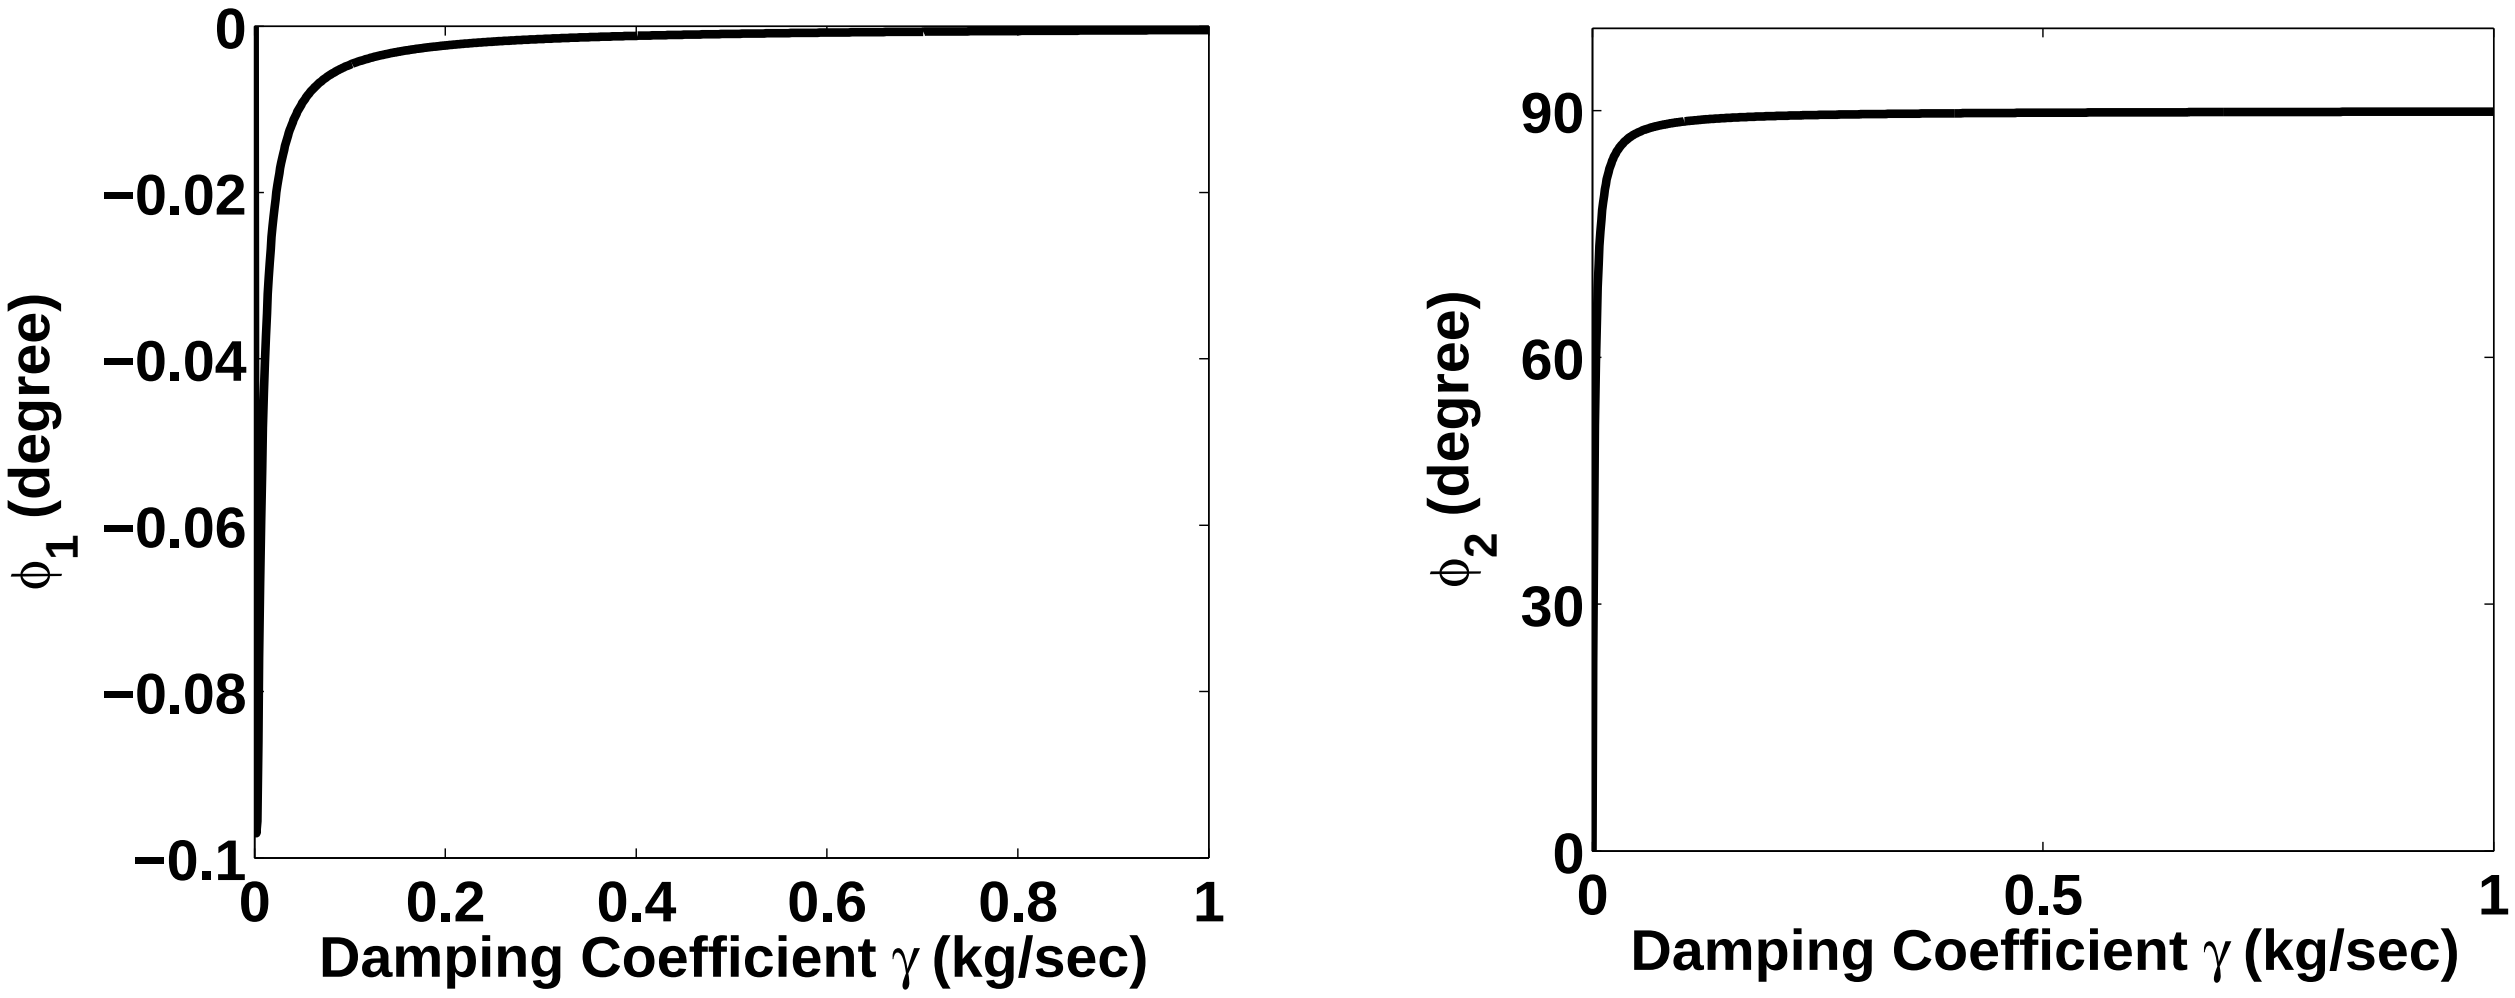

(a)

(b)

FIG. 4: Plots of ϕ_1 and ϕ_2 using equations (6) and (7), the . The following parameter values are used : $k_1 = 55090$N/m, $k_2 = 140$N/m, $m_1 = 2.2 \times 10^{-6}$kg, $m_2 = 2.7 \times 10^{-8}$kg and $\omega = 20$KHz(a) The phase ϕ_1 of the tuning fork and (b)the phase of the tip ϕ_2 with respect to the driver for different values of γ. Note that for Newtonian liquids with reasonable viscosity the ϕ_1 converges to zero and the ϕ_2 converges to 90 degrees, consistent with the ideas in conventional rheology.

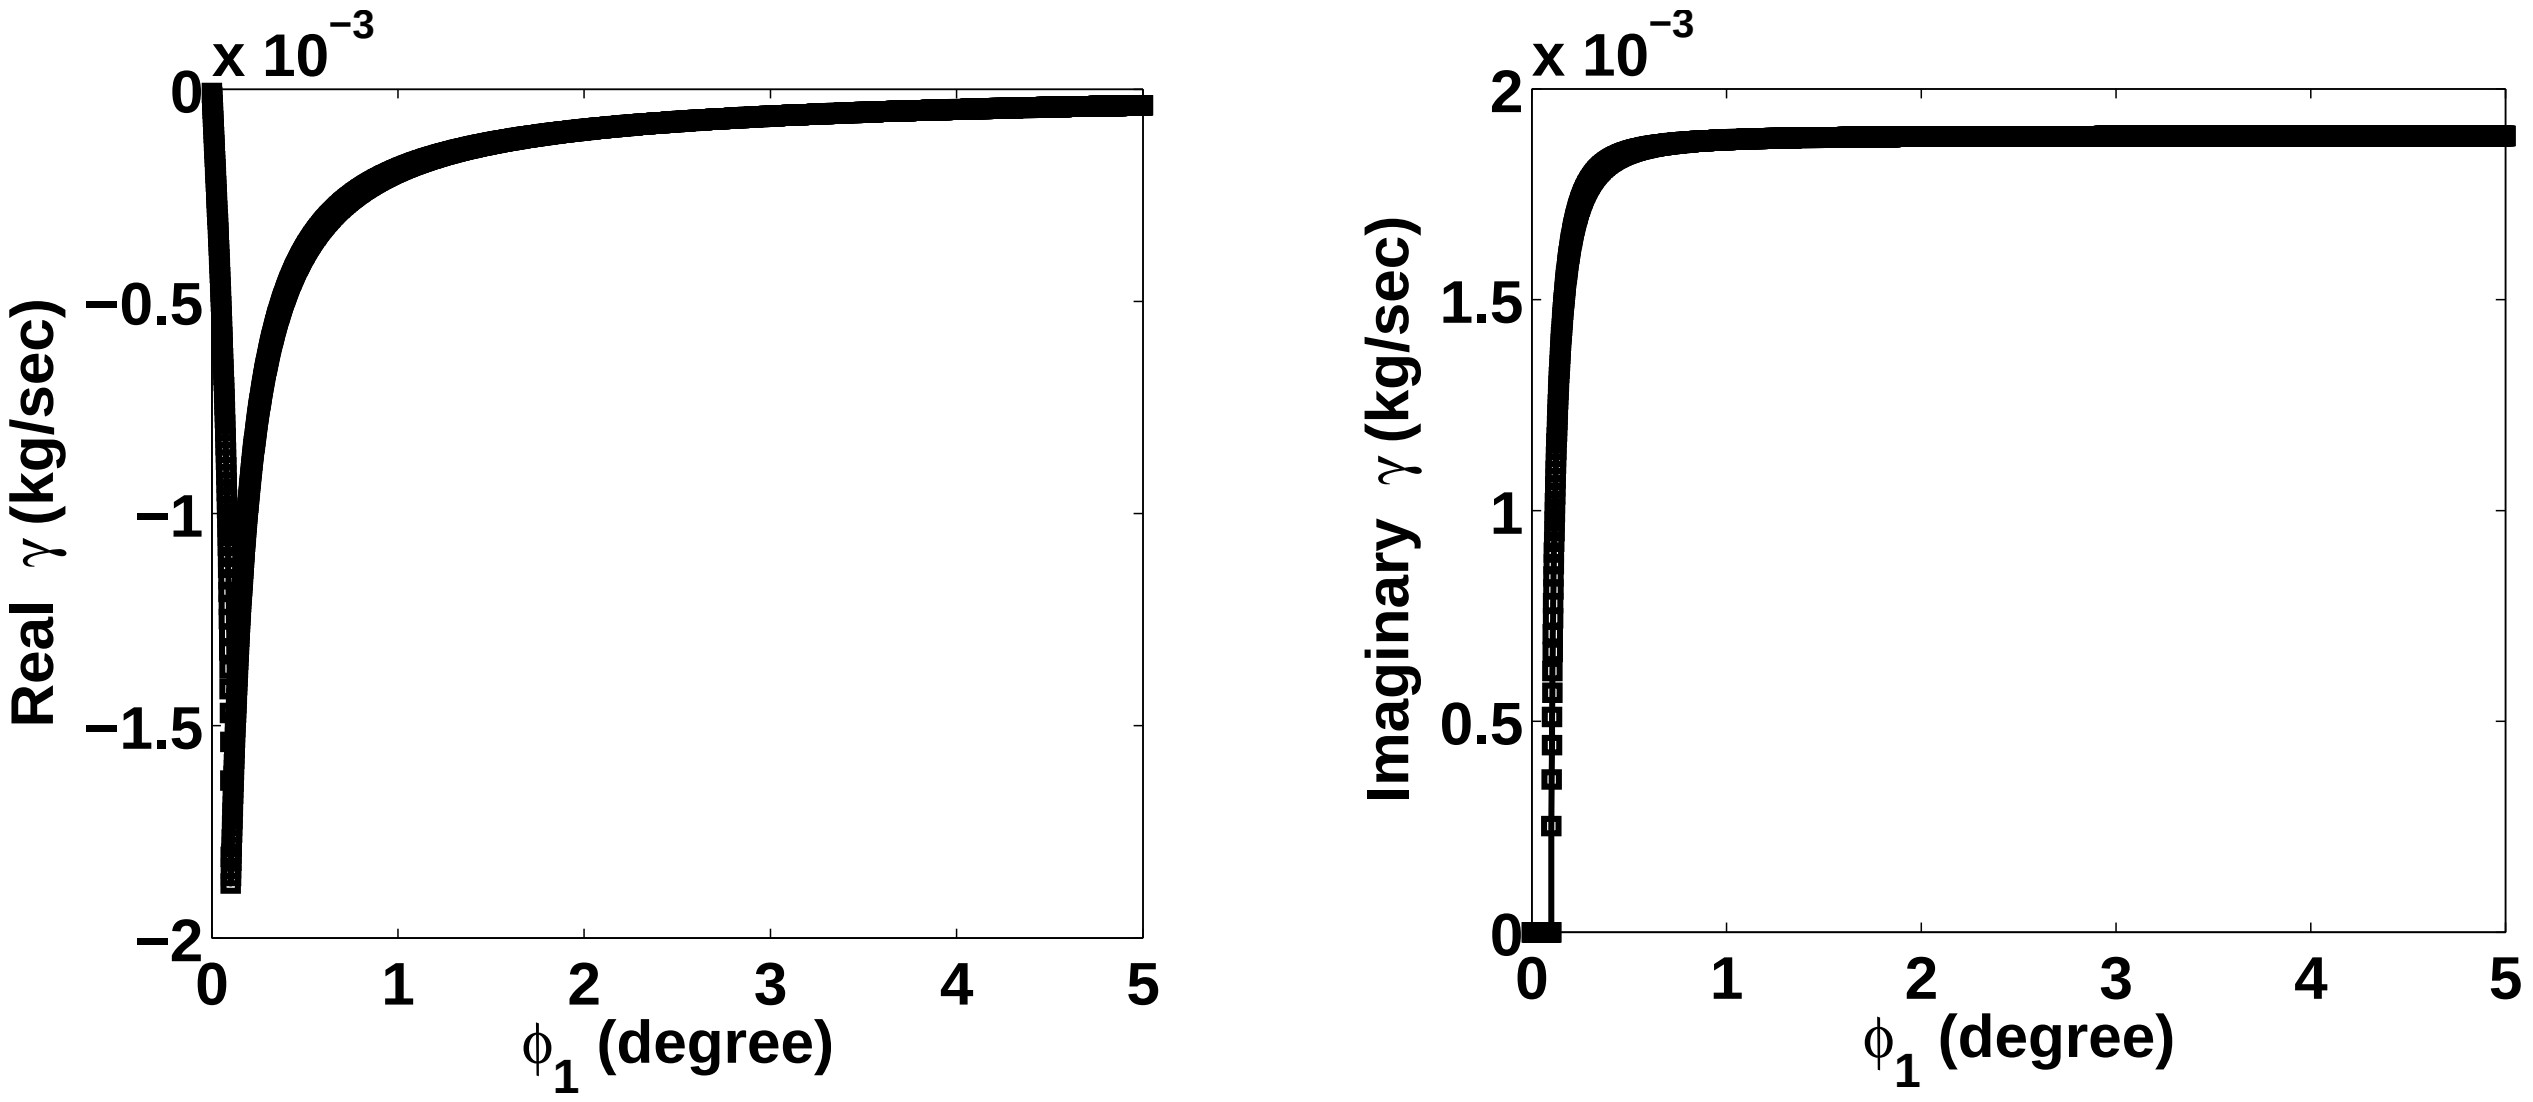

(a)

(b)

FIG. 5: The Real and Imaginary part of damping coefficient γ with increasing ϕ_1

III. THE INSTRUMENT

A. The force sensor

Tuning forks are procured from local market having following dimensions for each arm: length $L = 3.5$mm, width $w = 350\mu$m and thickness $t = 700\mu$ m with the electrodes covering the length $L_e = 3$mm. After carefully removing the tuning fork from its protection cap, we mount it on a piezo crystal to drive it mechanically as shown in figure 6. On resonance the free arm oscillates with much larger amplitude compared to the one sitting on the piezo-crystal and the difference in the charge accumulated due to strain in each arm is measured using a pre-amplifier as shown in the circuit diagram. A gain of 10^7 is used to convert these oscillations into measurable signal using a lock-in amplifier.



FIG. 6: Tuning Fork with fibre tip attached to the free arm

The resonance characteristic of the tuning fork without loading the fibre tip is measured. A typical quality factor of 800 is obtained for the operation in ambient environments. A single mode fibre with outer diameter of 127μm and core diameter of 9μm is pulled using a CO_2 laser based pipette puller to form a sharp tip. The fibre tip is then mounted on the free arm of the tuning fork as shown in the figure and the resonance characteristic is measured again to see the loading effects. Typically the resonance shift before and after mounting the fibre tip is 1-2 KHz. To estimate the amplitude of the free arm in nm from the measured signal in lock-in amplifier we use the geometry of the tuning fork and the piezoelectric modulus of quartz following[21]. The total charge developed per unit deflection of the free arm is:

$$q/z' = 12 d_{21} k_f L_e \left(\frac{L_e}{2} - L \right) / t^2$$

where d_{21} is the piezoelectric coupling constant.

The theoretical sensitivity is given by

$$S_{theory} \approx 2\pi f \times R \times q/z'.$$

For $f = 29284Hz$, and $R = 10M\Omega$ in our gain circuit

$$S_{theory} = 34.3635 \text{ mV/nm}.$$

B. The coarse and fine approach mechanism

The instrument is designed and built for shearing the nano-confined liquid between a sharp tip and a flat substrate. This requires the actuation of tip towards the substrate with precision of nm and the range of few mm.

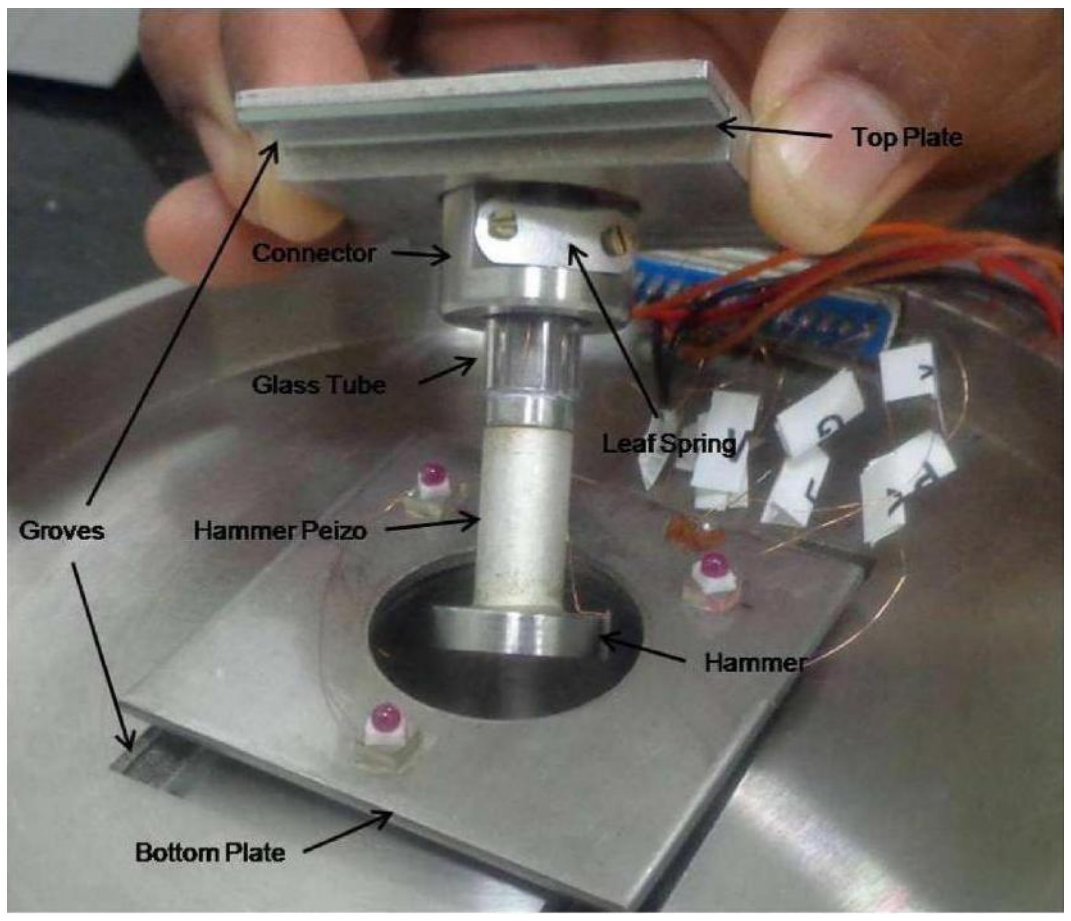

FIG. 7: A photograph showing the X-Y-Z coarse and fine approach mechanism

For approaching the fibre tip from separations of mm to nm we used the inertial sliding approach mechanism used first by D. Pohl [28], also discussed in detail in references [29] and [30]. The entire approach mechanism is placed in a heavy steel base where the central part is carved out to accommodate coarse and fine X-Y-Z positioner. To facilitate coarse motion a steel piece called hammer is attached to a piezo tube (hammer piezo). On top of the hammer piezo, a quartz glass tube is fitted. This tube is inserted in a connector having a copper leaf spring that holds quartz tube. The tension in the leaf spring can be adjusted to serve the controlled vertical sliding of the tube against gravity. The quartz tube makes contact with the connector piece along flat walls. Electrical pulses with slowly rising edge and fast drop off are applied to the hammer piezo. During the initial slow rising of the pulse, the hammer piezo expands (contracts) moving the hammer up (down) and the tube remains clamped at the leaf spring. When the voltage suddenly drops to zero, the hammer remains in its place due to inertia pushing the tube up (down) achieving a net movement in each pulse. The height and width of the pulse can be controlled to achieve the desired step length, typically tens of nm. The connector bearing the quartz tube is fixed onto a coarse X-Y scanner. The quadrant piezo tube (scanner piezo) is mounted inside the quartz tube and moves with the hammer piezo, hammer and the quartz tube assembly. A liquid cell is magnetically attached on the top of the scanner tube. The cell comprises of two circular Teflon pieces clamped together with a Viton O-ring between them. The top Teflon piece has an opening to allow access to the fibre tip mounted on the Tuning Fork. The liquid is filled in the cell from the top opening with a glass syringe.

The coarse X-Y positioning of the sample also uses inertial sliding principle. The X-Y positioner consists of a heavy steel plate called top plate in the figure 7. The top plate has grooves cut out in it for X motion. Similarly, the grooves are cut in a perpendicular direction in the instrument base for Y motion. These grooves are seen in Figure 7. Shear piezos in alignment with the grooves are glued on both sides of the middle plate. Ruby balls are glued in the recesses formed on macor pieces that sit on the shear piezos. For X-Y motion, the slow rising and fast falling pulses are applied to shear piezos similar to Z coarse motion described previously. The central part of both the top and middle plates has a circular hole for the passage of the Z-coarse positioner and the scanner. The connector holding the Z positioner is mounted on the top X-Y plate as shown in Figure 7. All the actuation signals and the feedback loop are generated using LabView. National Instruments data acquisition card (PXI-6259) is used for interfacing the instrument with the computer.We calibrated the Z-scanner piezo after mounting the liquid cell using a Michelson Morley interferometer. This gives the sensitivity of the Z-scanner as 18 nm/V. A circular plate with a hole on the top is used to cover the entire approach mechanism assembly. The AFM base is kept on an active vibration isolation table from Accurion, micro series model.

IV. MEASUREMENT METHODOLOGY

In order to keep the tuning fork out of the liquid we attach a fibre to its free arm so that the fibre tip extends 2 to 3mm out from the fork and the tip end of the fibre remains immersed in the liquid as shown in the figure 1. Freshly cleaved mica is clamped below the Viton O- ring of the liquid cell and the cell is immediately filled with Millipore water. The fibre with tip at its end is slowly lowered into the liquid using coarse Z-motion. The change in amplitude upon engaging with surface is largest on resonance. We use this fact for engaging the tip with the surface. The tuning fork is oscillated on resonance and the tip is approached towards the surface in auto-approach mode. A set of pulses are applied to the hammer piezo and between two successive sets the scanner piezo expands its full range to confirm if the desired set-point is reached. After reaching the set-point amplitude, the pulses are stopped and the scanner piezo is retracted back fully. The whole procedure is repeated with sets having smaller number of pulses and lesser pulse height in order to bring the engagement point close to zero Z-voltage on the scanner piezo. This ensures that the tip-substrate engagement point is always within reach while acquiring the data. The tuning fork is now oscillated below the resonance and the fibre is approached and retracted.The rheological response of the nano-confined liquid between the tip and the atomically smooth substrate as the tip is progressively approached towards substrate is inferred by measuring the phase lag and amplitude change in the tuning fork arm. Using lock-in amplifier the amplitude and phase of the arm of the tuning fork carrying the fibre is measured. The change in amplitude with respect to the normal position of the tip from the surface gives us the change in force the tip is experiencing compared to the bulk. Figure 8 (a) shows that the amplitude decreases upon approach within about 5 nm from the surface. This reduction in amplitude indicates larger drag force upon confinement. Figure 8 (b) shows the phase ϕ_1 versus the separation.

V. RESULTS AND DISCUSSION

As discussed in section II, the phase relationship between applied sinusoidal force and the tuning fork's free arm can give us the nature of the nano-confined liquid. Any possible phase difference between these two is a indication of a non-Newtonian behaviour. Figure 8 shows that there is finite phase change upon approaching the tip within about 5 nm from the substrate. In AFM experiments, the zero of the tip-substrate separation is decided by the sudden increase in the normal amplitude of the cantilever[20]. In our set-up the normal stiffness of the tuning fork- fibre

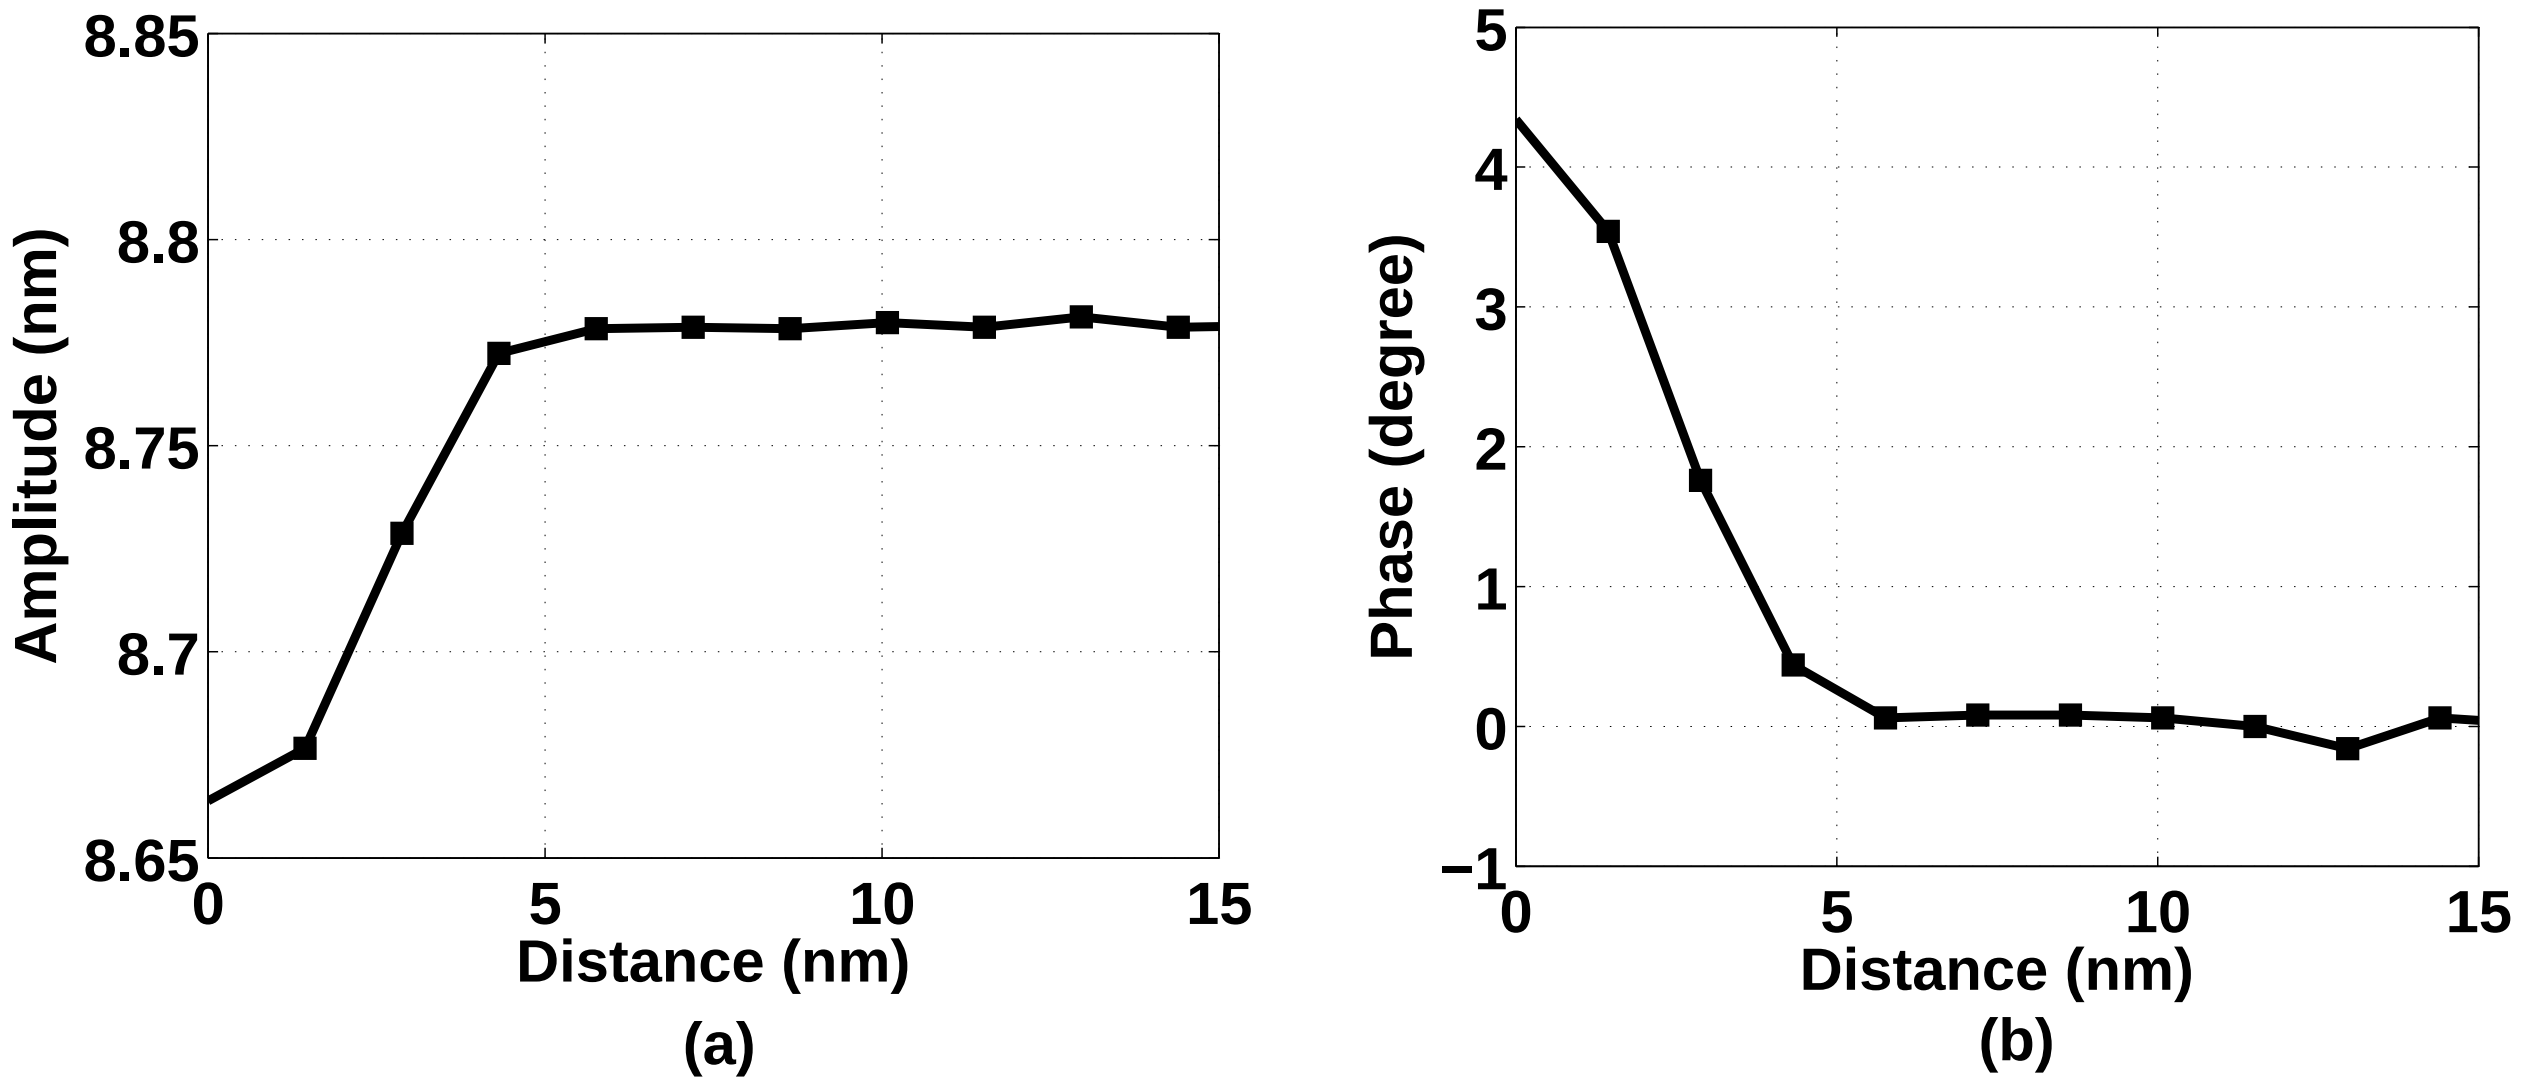

FIG. 8: The (a)Amplitude and (b)Phase of the tuning fork with separation at 12 KHz shear frequency.

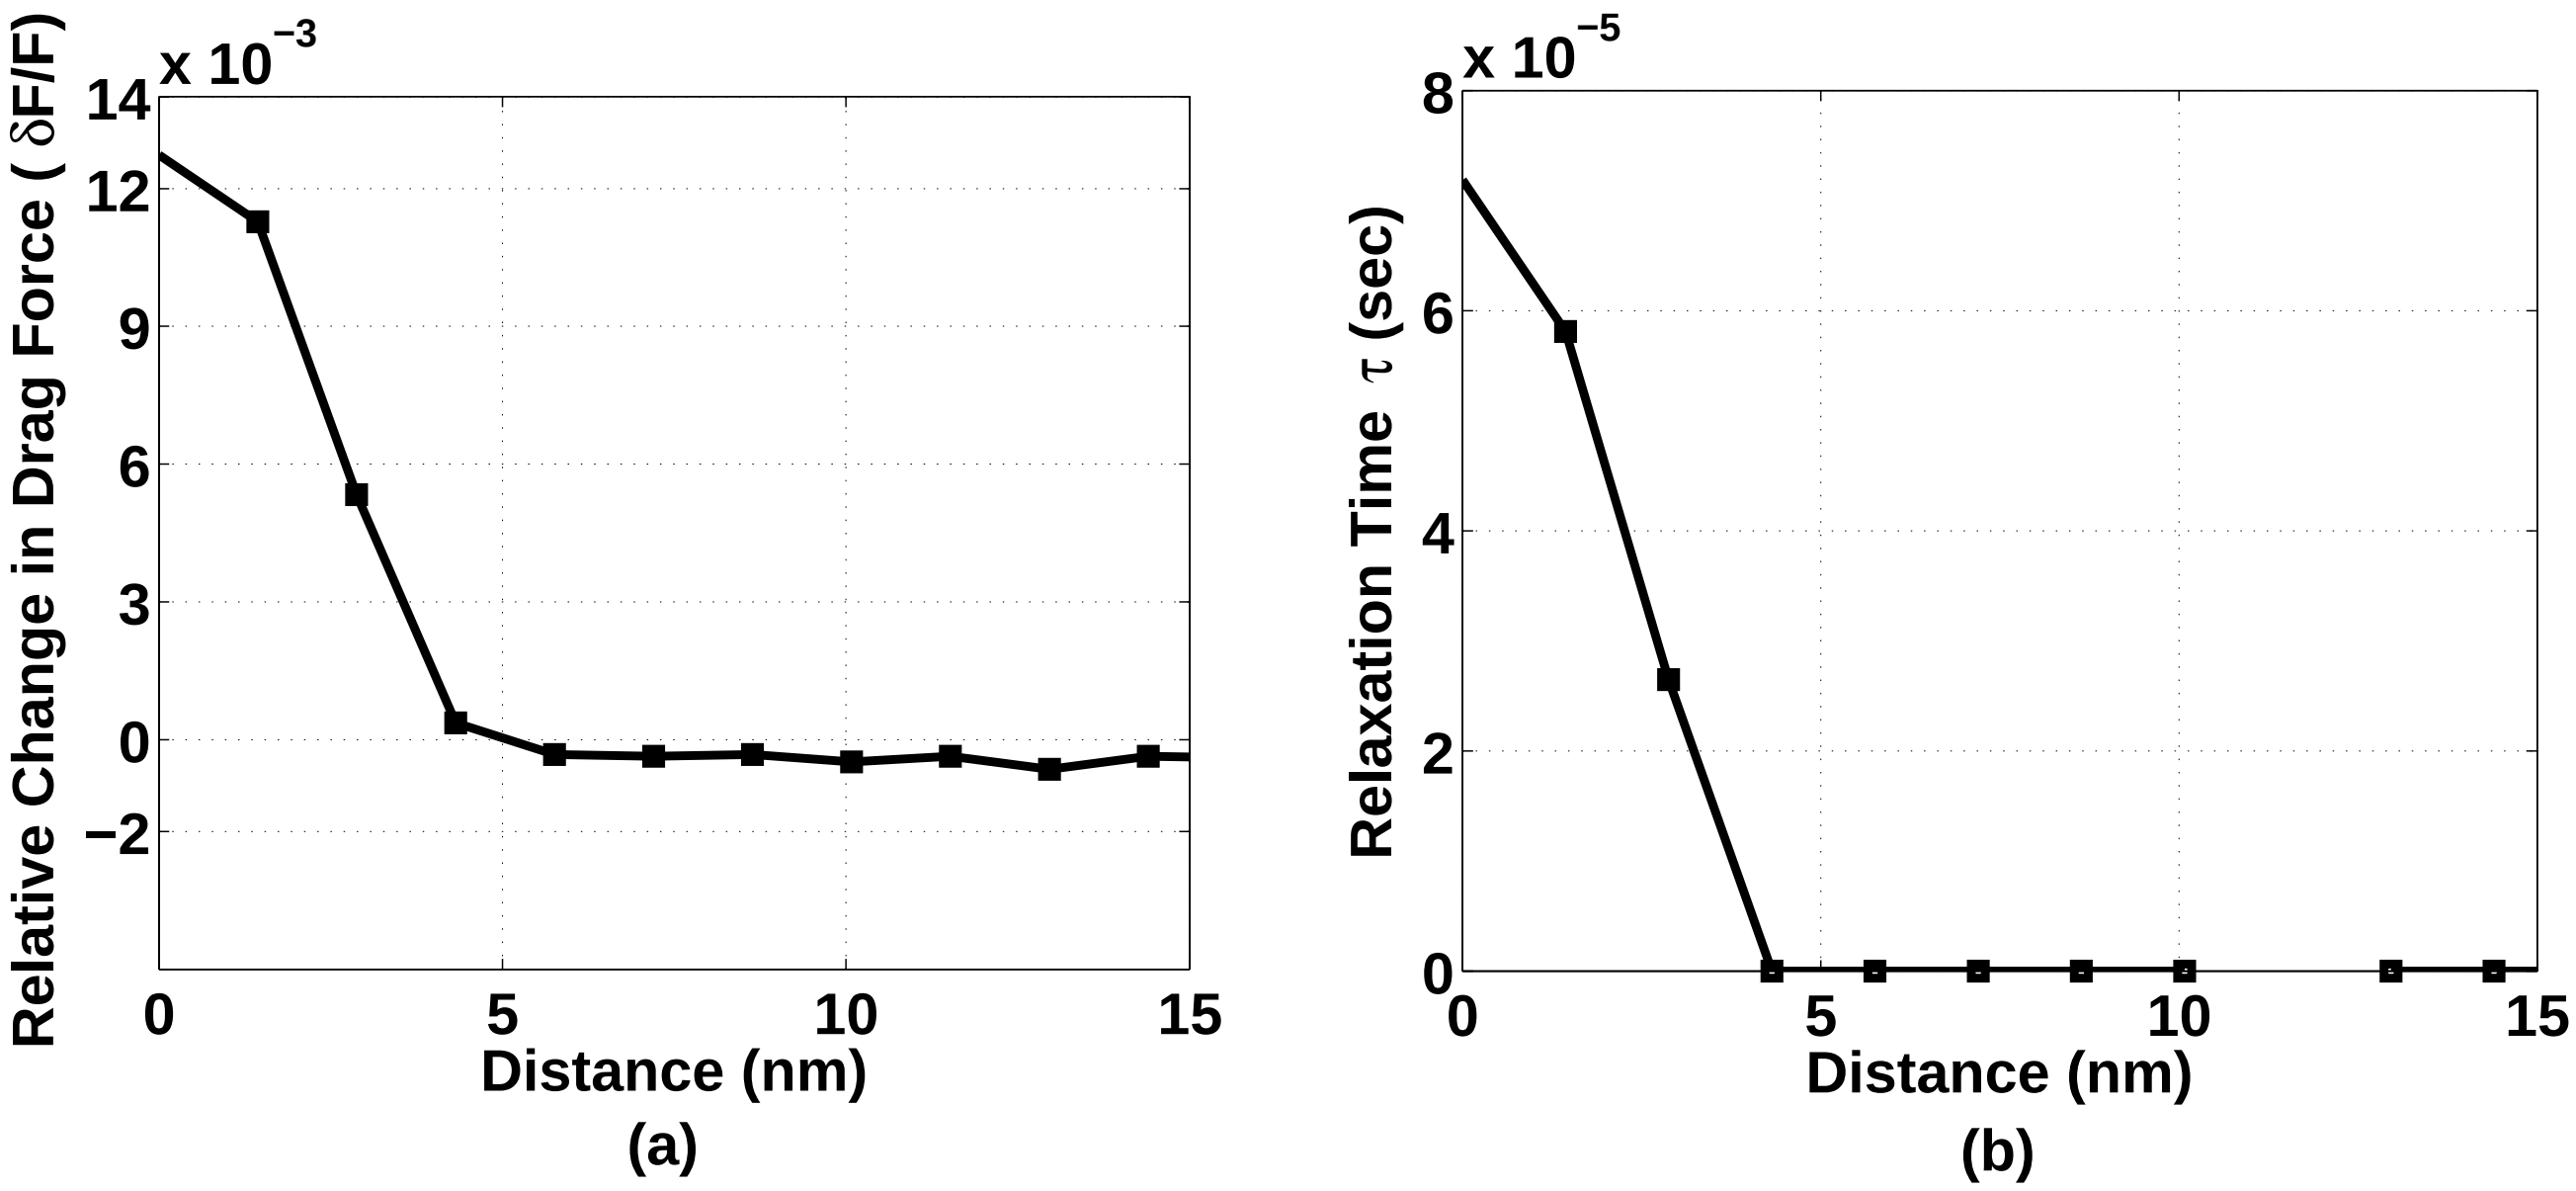

FIG. 9: (a) The fraction change in drag force upon confinement from the bulk viscous drag, and (b)Relaxation time τ with separation at 12 KHz shear frequency

system is nearly infinite. We observe that the amplitude does not vary much after making a hard contact with the surface, this possibly means that the last layer of liquid on the surface is not drained out and provides a constant drag to the oscillating tip. The zero of the tip-substrate separation in our experiments is decided by considering the percentage change in the amplitude after the engagement. Using equation [6], the phase data is converted into real and imaginary part of damping coefficient. Equation(8) is used to plot relaxation time versus separation. Figure 9(a) shows a plot of relaxation time versus separation for a water at 12 KHz of shear frequency. The relaxation increases significantly compared to bulk water and is measurable under the shear at 12 KHz. It attains a value between 0.01 and 0.1 ms when the film thickness is less than 5 nm, a value comparable to the one measured using the shear and normal measurements using AFM [19, 20]. In these experiments the relaxation as well as drag force is measurable only below 1 nm of film thickness. This is possibly because the confining areas under AFM tip are much smaller compared to the present measurements and films with thickness above 1 nm offer immeasurably low change in drag force compared to the bulk viscous drag. Figure 9 (b) shows the relative change in the drag force when the tip is oscillating close to the substrate. It is instructive that the change in drag force offered by the nano-confined volume of the liquid is only 2 to 8 percent of the bulk drag and will not have a discernible effect if the thermal noise in the force measurement is not low enough. By comparing the drag force and the relaxation time one can infer various regimes of non-Newtonian behaviour of the nano-confined liquid such as viscoelastic or shear thinning. The off resonance operation ensures that the measurements can be performed over a range of shear amplitudes and frequencies.

VI. ACKNOWLEDGEMENT

The authors would like to thank Arijit Bhattacharyay for useful discussions. The work is funded in part by Department of Science and Technology (DST) nano-science unit grant (SR/NM/NS-42/2009) and IISER-Pune.

---

[1] Finney J.L. Finney, Farad. Discuss. 103, 1-18 (1996).
[2] J. Israelchvili Intermolecular and surface forces (Academic Press, London, 1992).
[3] B.J. Persson, Sliding friction: Physical Principles and Applications (Springer, Heidelberg, 2000), $2^n d$ ed.
[4] Granick, S. and Bae,C. **322**, 1477-78 (2008).
[5] Mingyan He, Amy Szuchmacher Blum, Gregor Overney, and Ren M. Overney, Phys. Rev. Lett. **88**, 154302 (2002).
[6] Ashis Mukhopadhyay, Jiang Zhao, Sung Chul Bae, and Steve Granick, Phys. Rev. Lett. **89** 136103(2002).
[7] S. Granick, Science **253**, 1374 (1991).
[8] Tai-De Li, Jianping Gao, Robert Szoszkiewicz, Uzi Landman and Elisa Riedo Phys. Rev. B. **75**, 115415 (2007).
[9] Eugenia Kumachevaa and Jacob Klein J. Chem. Phys. **108**, 7010 (1998).
[10] R.G. Horn and J. N. Israelchvili, J. Chem. Phys. **75**, 1400, (1981).
[11] S. Granick, S. Bae, S. Kumar and C. Yu, Physics **3**, 73(2010).
[12] H.K.Christenson, D. W. R. Gruen, R. G. Horn and J. N. Israelchvili *ibid* **87**,1834(1987).
[13] B. V. Derjaguin and N.V. Churaev Langmuir **3**, 607(1987).
[14] R. G. Horn, D. T, Smith and W. Haller Chem. Phys. Lett. **162**, 404 (1989).
[15] J. N. Israelchvili, J. Colloid interface Sci. **263**, 110 (1986)
[16] Zhu,Y. and Granick, S. Phys. Rev. Lett. **87**, 096104-9 (2001).
[17] Raviv, U. , Laurat, P. Klein, J. Nature **413**, 51-54 (2001).
[18] Raviv, U Klein, J. Science **297**, 1540-43 (2002).
[19] Li, T.D. Reido, E. Phys. Rev. Lett. **100**, 106102-4 (2008).
[20] Khan, S. H., Matei, G., Patil, S. and Hoffmann, P.M. Phys. Rev. Lett. **105**, 106101(2010).
[21] F. Giessibl Appl. Phys. Lett. **76**, 1470 (2000).
[22] M. Lee, J. Jahng, K. Kim and W. Jhe, Appl. Phys. Lett. **91** 023117 (2007).
[23] F. Giessibl, S. Hembacher, H. Bielefeldt, J. Mannhart Science **289**, 422(2000)
[24] L. Gross, F. Mohn, N. Moll, P. Liljeroth and G. Meyer Science, **325** 1110 (2009).
[25] Markus Ternes, Christopher P. Lutz, Cyrus F. Hirjibehedin, Franz J. Giessibl and Andreas J. Heinrich science **319**, 1066 (2008).
[26] H. Barnes, J. F. Hutton and K. Walters, *An Introduction to Rheology*, (Elsvier, 1998), p.46-48
[27] R. G. Larson, *Structure and properties of complex fluid* (Oxford University Press, 1998), p. 13
[28] D. W. Pohl, Rev. Sci. Intrum **58**, 54 (1987).
[29] B. L. Blackford and M. H. Jericho Rev. Sci. Instrum., **68**, 134(1997).
[30] S. Patil, G. Matei, H. Dong, P. M. Hoffmann, M. Karakse and A. Oral Rev. Sci. Instru. **76**, 103705 (2005).